



Black Magnetic Needle Counters

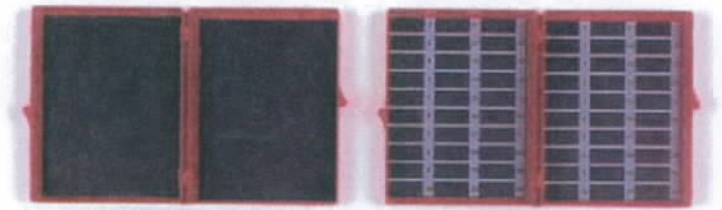

70561

70560

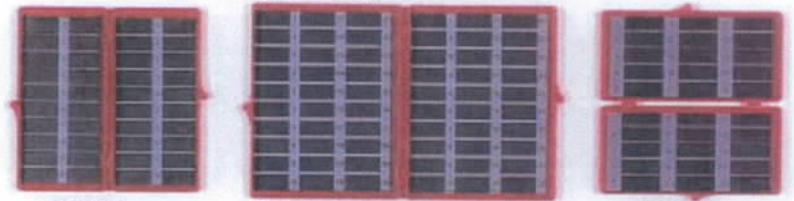


70120

70160


70130




70424




70131



70930




70110

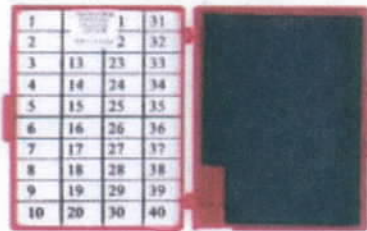


70514




70660

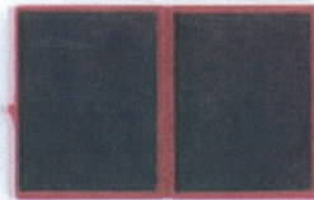


70960

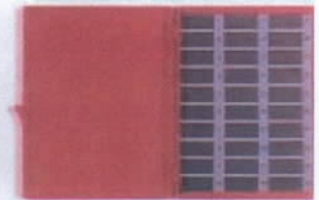

70161

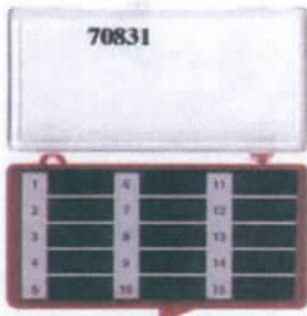


70831

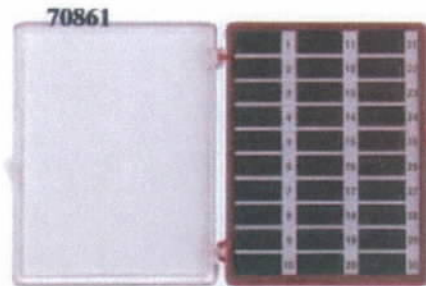

70861




70730

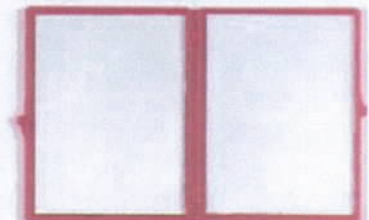

70761



70760



70731

White Magnetic Needle Counters

Syringe Transfer Cup




80100

70514y



■ Foam Strip Needle Counters

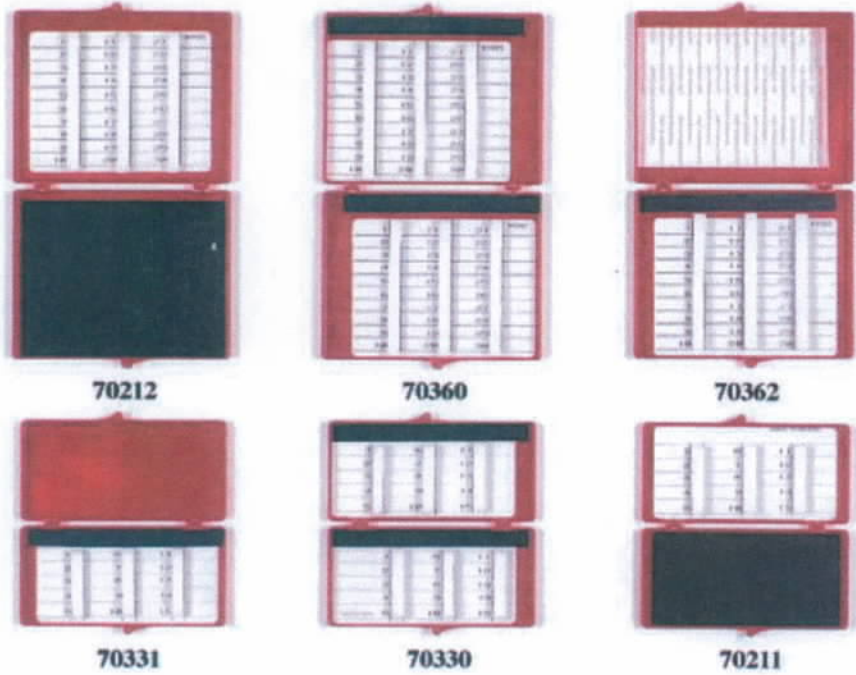

70212

70360

70362

70331

70330

70211


■ Foam Block Needle Counters



70423

70412


70440

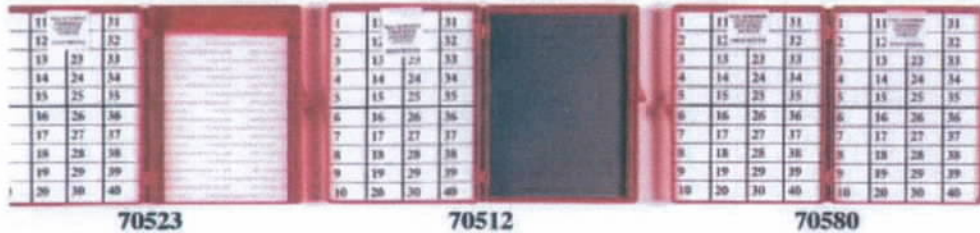

70523


70512

70580

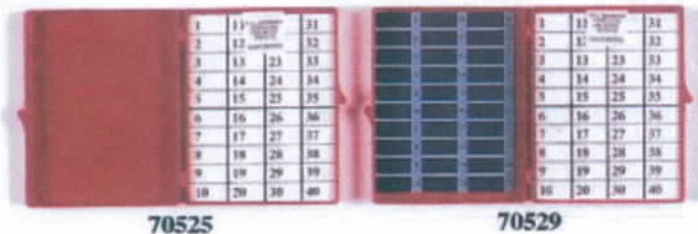

70525

70529

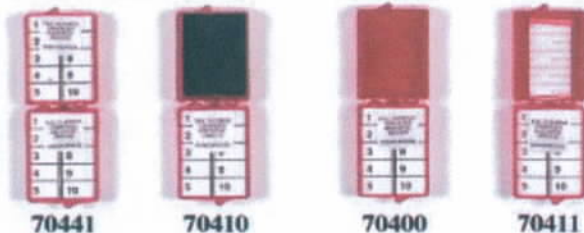

70441

70410


70400

70411

- Latex Free
- Meets OSHA Requirements
- Available Sterile or Non-Sterile
- Ask for our Needle Counters in your Custom Trays & Packs

All needle counters not pictured

■ Needle Counter with Blade Remover and Locking Closure

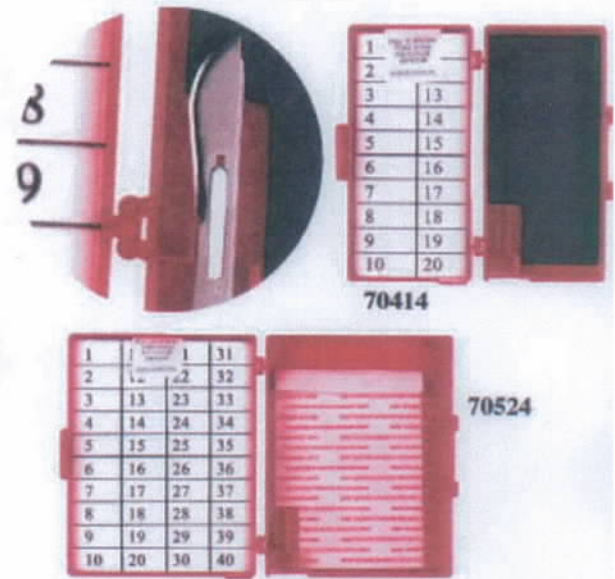


70414




70524

■ Magnetic Needle Counters with Clear Lid

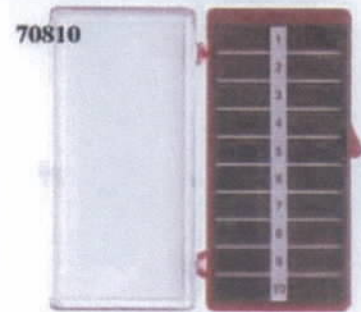

70810

■ Yellow Needle Counters with Blade Removers

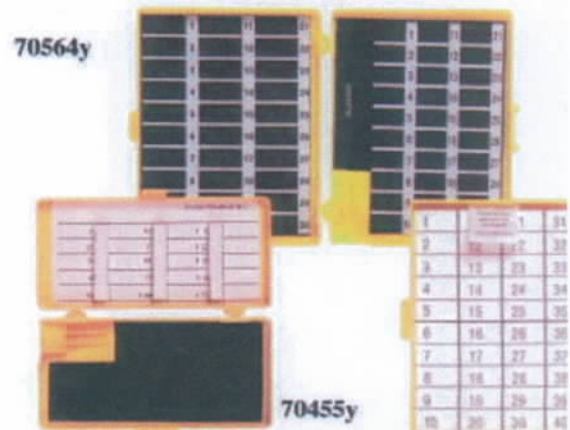


70564y

70455y



SAF-T PASS™ TRANSFER DRAPE

SAFE INSTRUMENT & SHARPS TRANSFER

- complies with OSHA requirements (29 CFR 1910.1030; CPL 2.103) and JCAHO standards to reduce accidental sharps injuries
- OSHA states "proper work practices (e.g., no-hands procedures in handling contaminated sharps, eliminating hand-to-hand instrument passing in the operating room)"

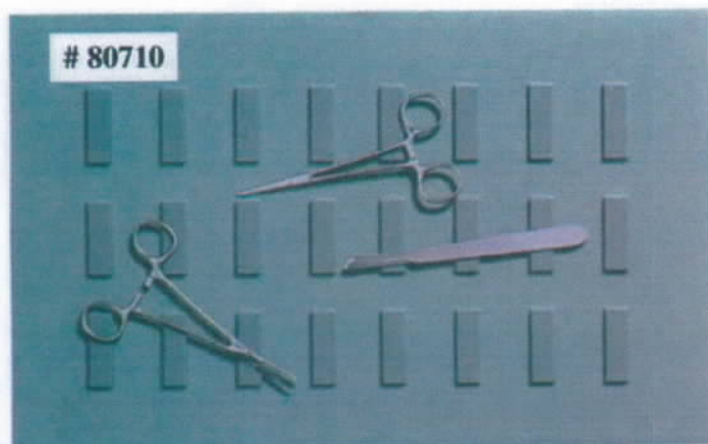

- magnetic and non-magnetic transfer drapes facilitate "hands-free" neutral zone passing.
- flexible; conforms to any shape or position
- single use; cost effective
- 100% non-magnetic with weighted edges

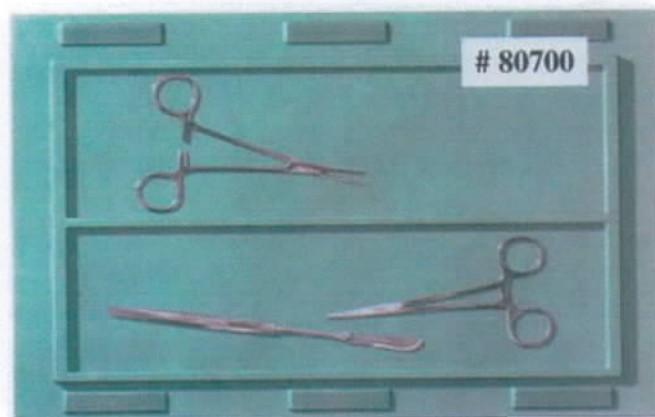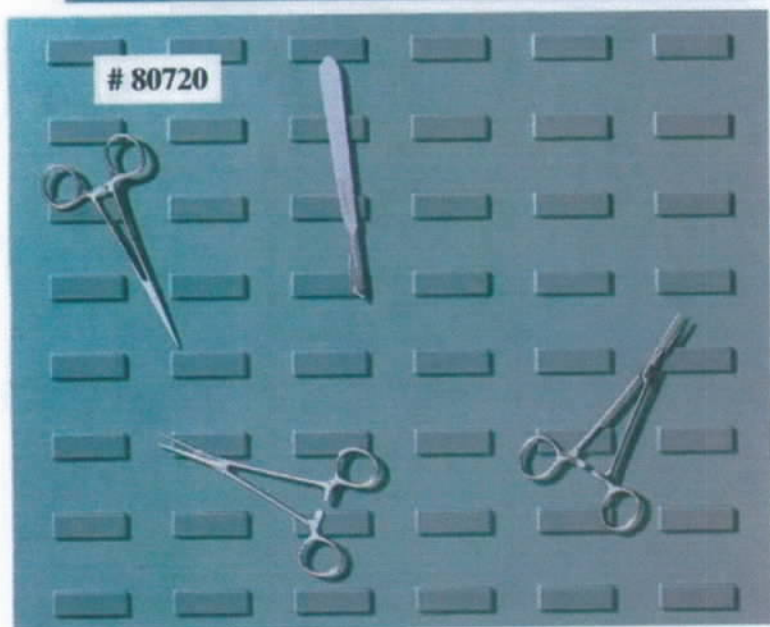

<i>Product</i>	<i>Reorder #</i>
Magnetic 16" x 10"	80710
Magnetic 16" x 20"	80720
Non-Magnetic w/Trays 16" x 10"	80700

Ask for our
SAF-T Pass™ Transfer Drapes
in your Custom Trays & Packs



SAF-T PASS™ REUSABLE TRANSFER ZONE

SAFE INSTRUMENT & SHARPS TRANSFER

80855

■ complies with OSHA requirements (29 CFR 1910.1030; CPL 2.103) and JCAHO standards to reduce accidental sharps injuries

■ provides neutral zone for safe "hands-free" passing of instruments

■ reusable; cost effective; sterilization by ETO or steam

80856

■ available with non-magnetic neutral transfer zone

■ safe and effective transfer between staff and surgeon

■ flexible; conforms to any shape or position

80885

80886

<i>Product</i>	<i>Case Quantity</i>	<i>Reorder #</i>
12" x 8"	3	80855
12" x 8" w/transfer zone	3	80856
12" x 16"	3	80885
12" x 16" w/transfer zone	3	80886

